


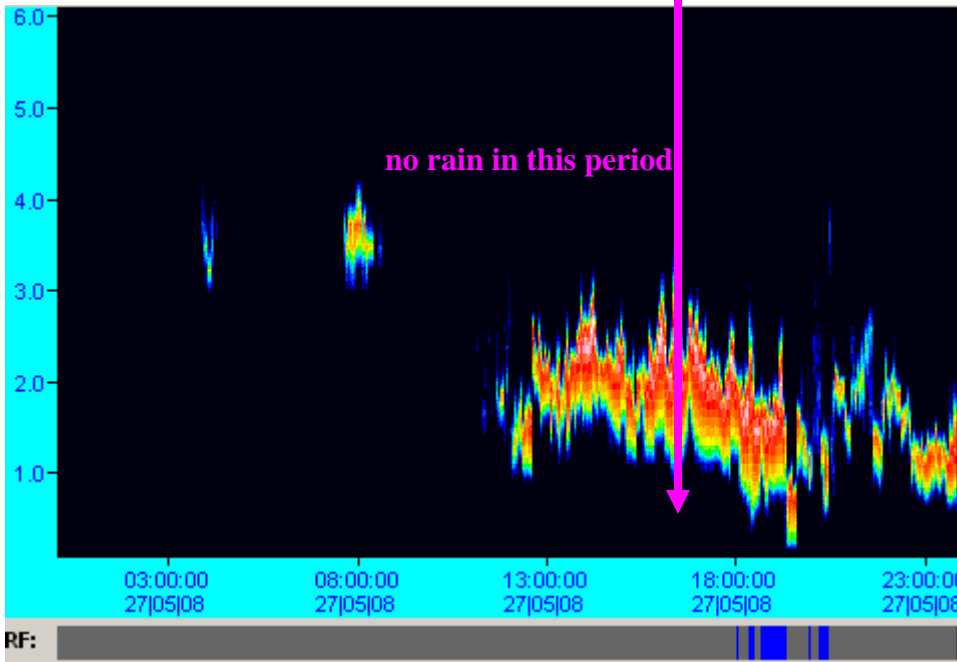
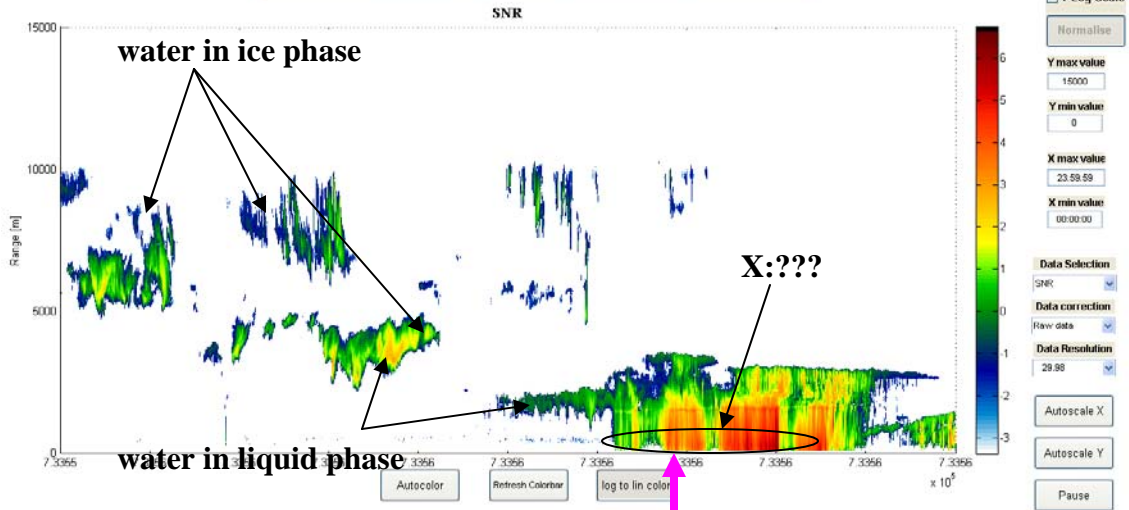



Measurement: 20080527_0000-080527_235955-02-01.mtf

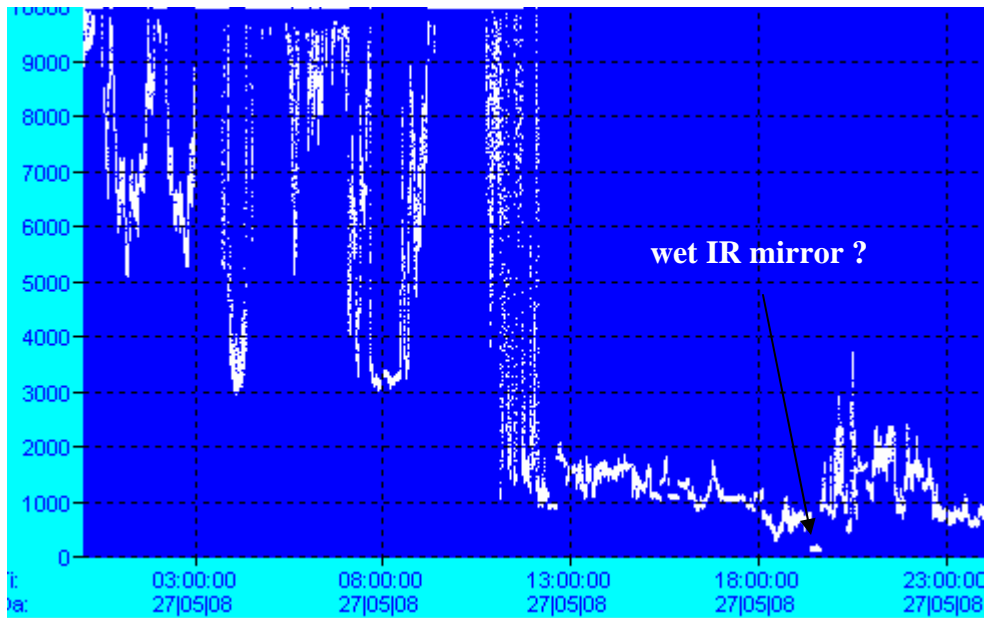

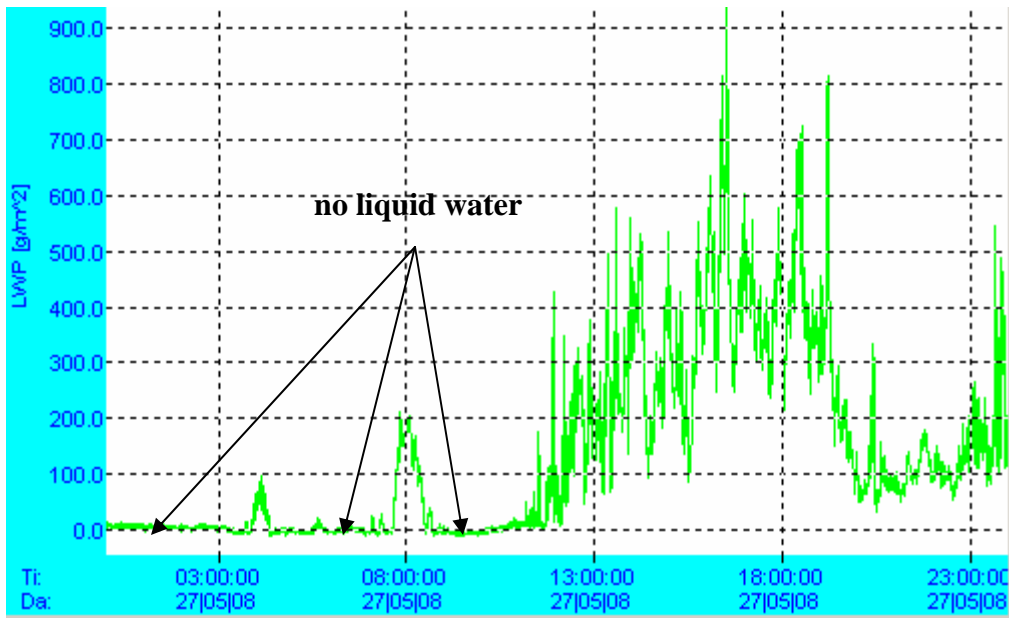


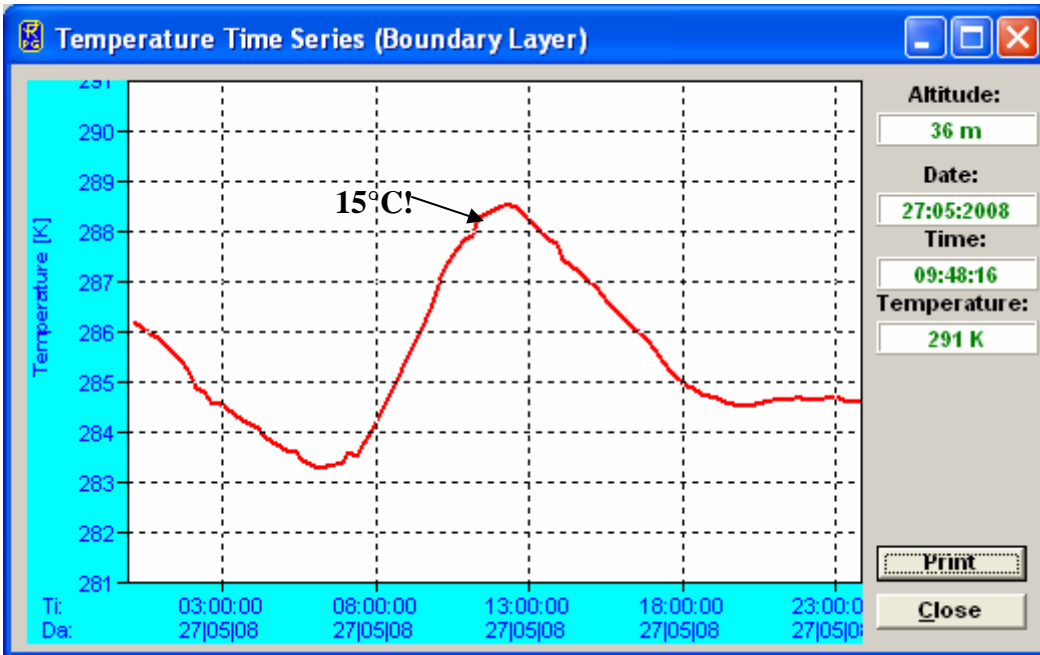

Temperature time series measured by the BL profiling method close to the ground

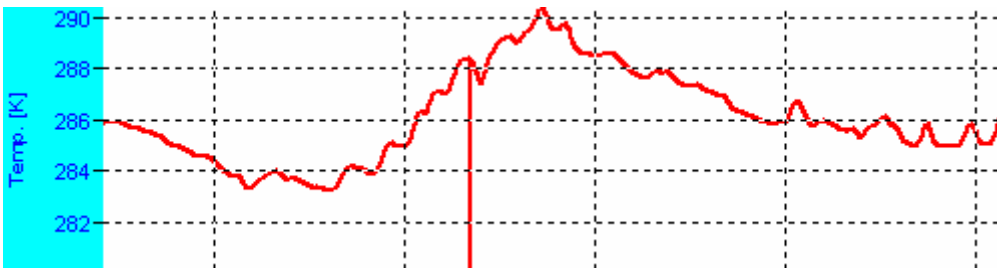

Temperature time series measured by the surface sensor. The two time series agree very well with each other.

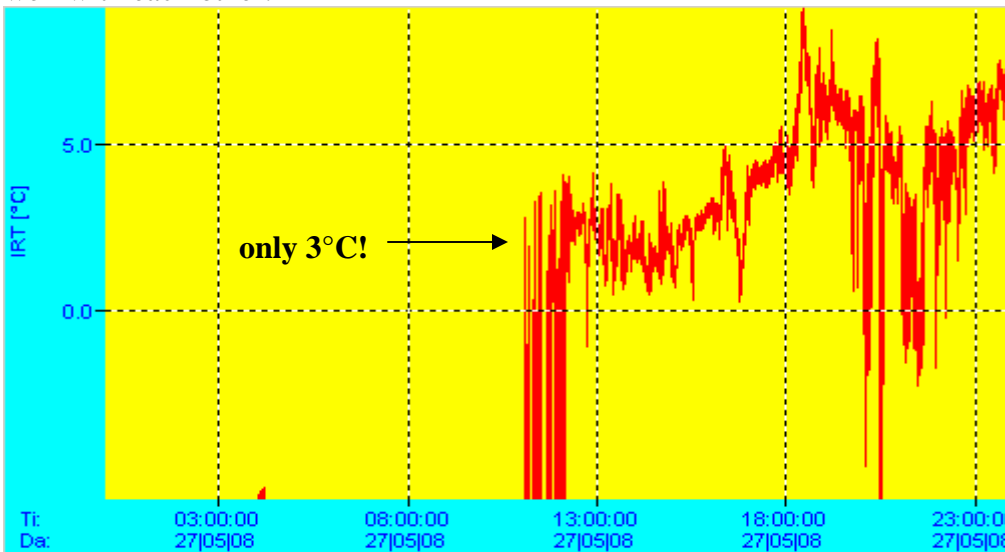

IR temp. is always significantly lower than surface temp. Therefore the CBH cannot be very low.

drizzle (virga), these are rain droplets that never reach the ground!

